



Lead
Stream water




Pb
ICP-MS, detection limit $0.005 \mu\text{g l}^{-1}$
Number of samples 807
Median $0.093 \mu\text{g l}^{-1}$

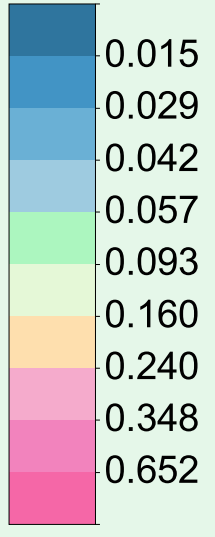

Pb $\mu\text{g l}^{-1}$

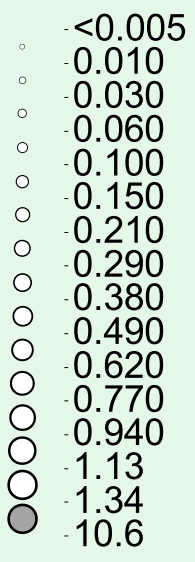

FOREGS
Geochemical Baseline Mapping

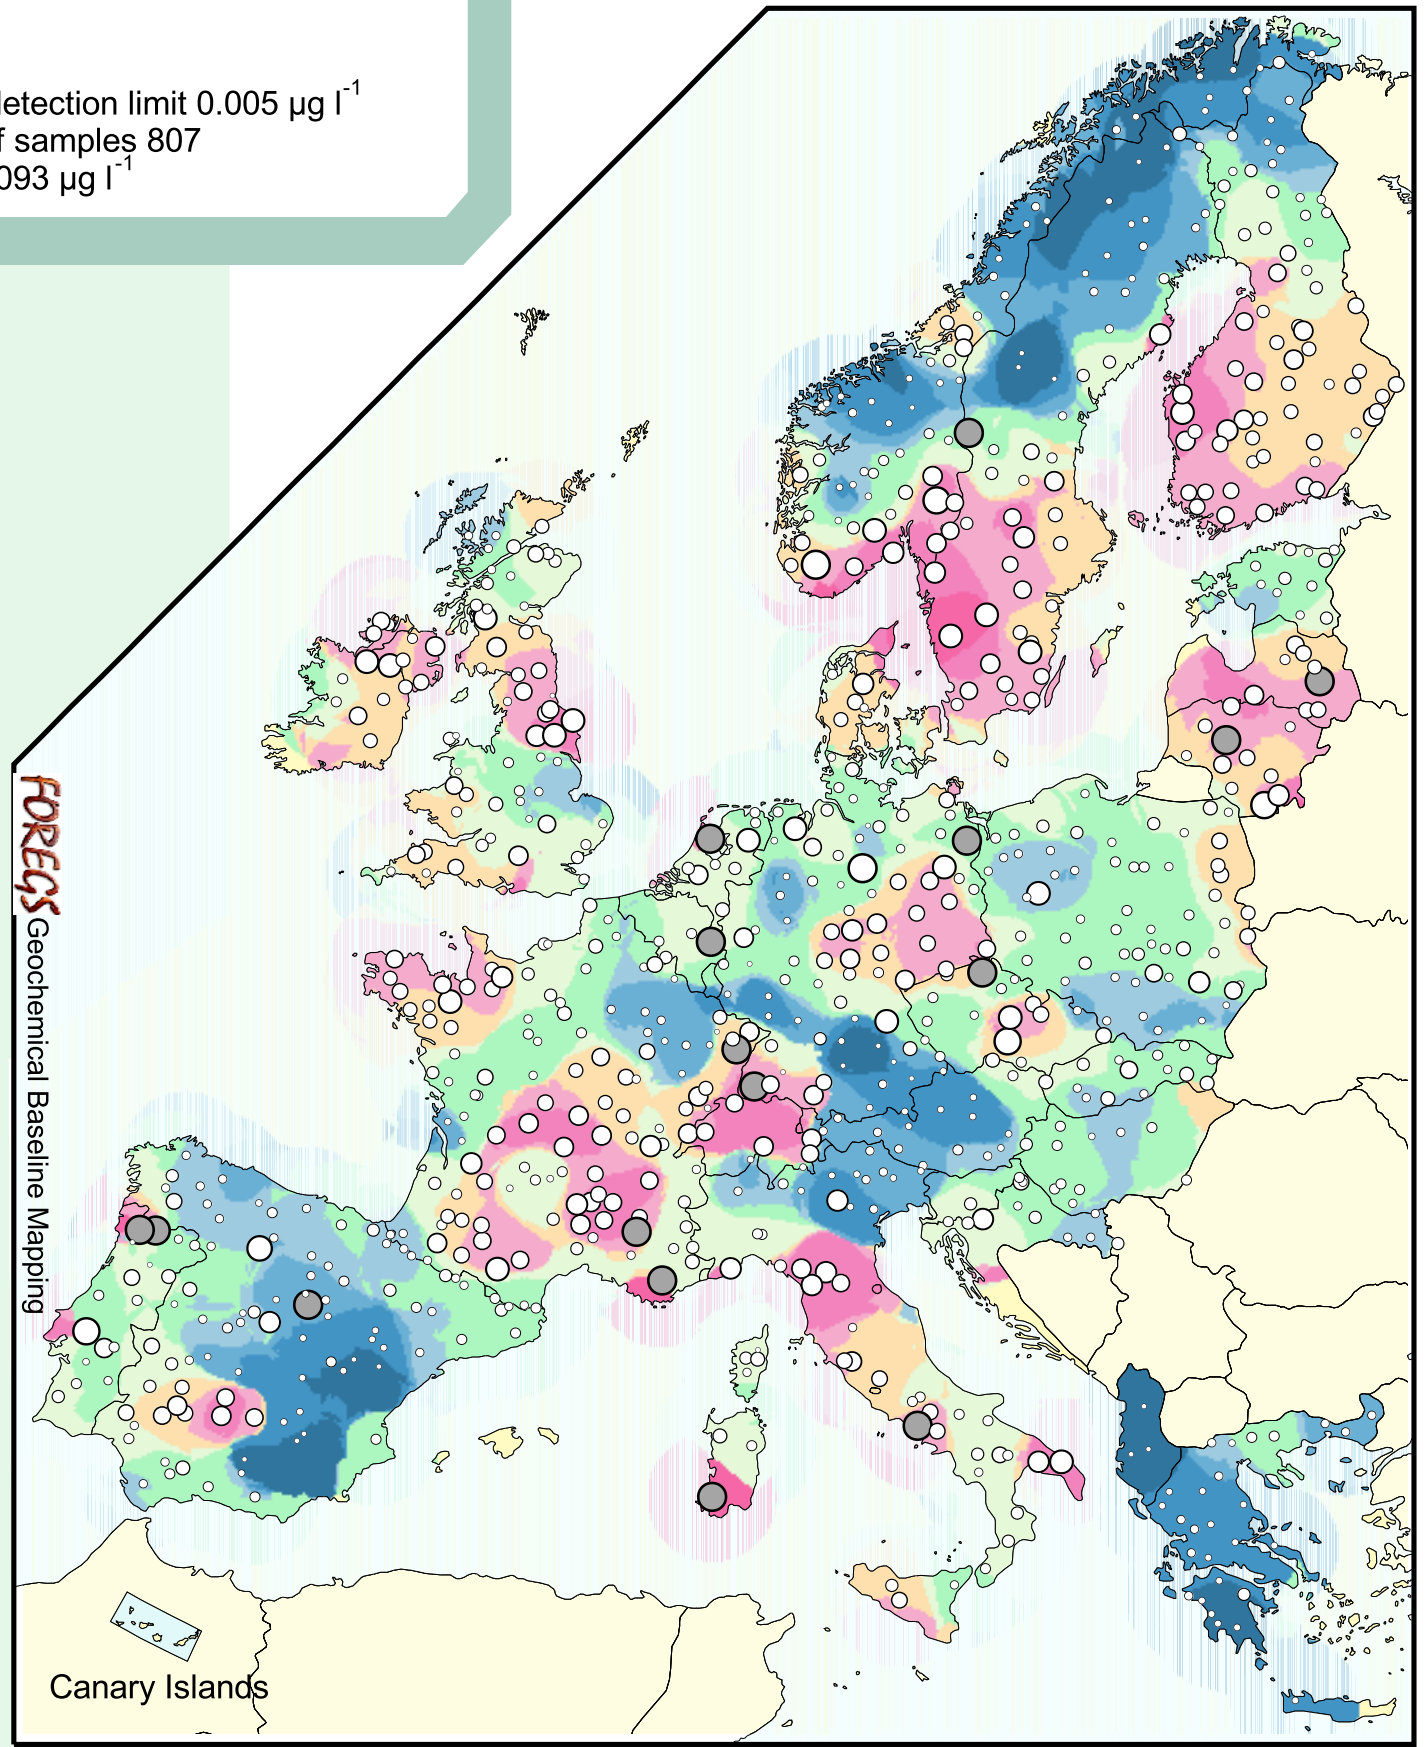

Canary Islands